


ZP\_HMQCGP\_3h CDC13 {C:\Bruker\TopSpin3.6.0} AMP 15



Current Data Parameters  
NAME CCY\_55\_06-ppdoLavHex  
EXPNO 12  
PROCNO 1

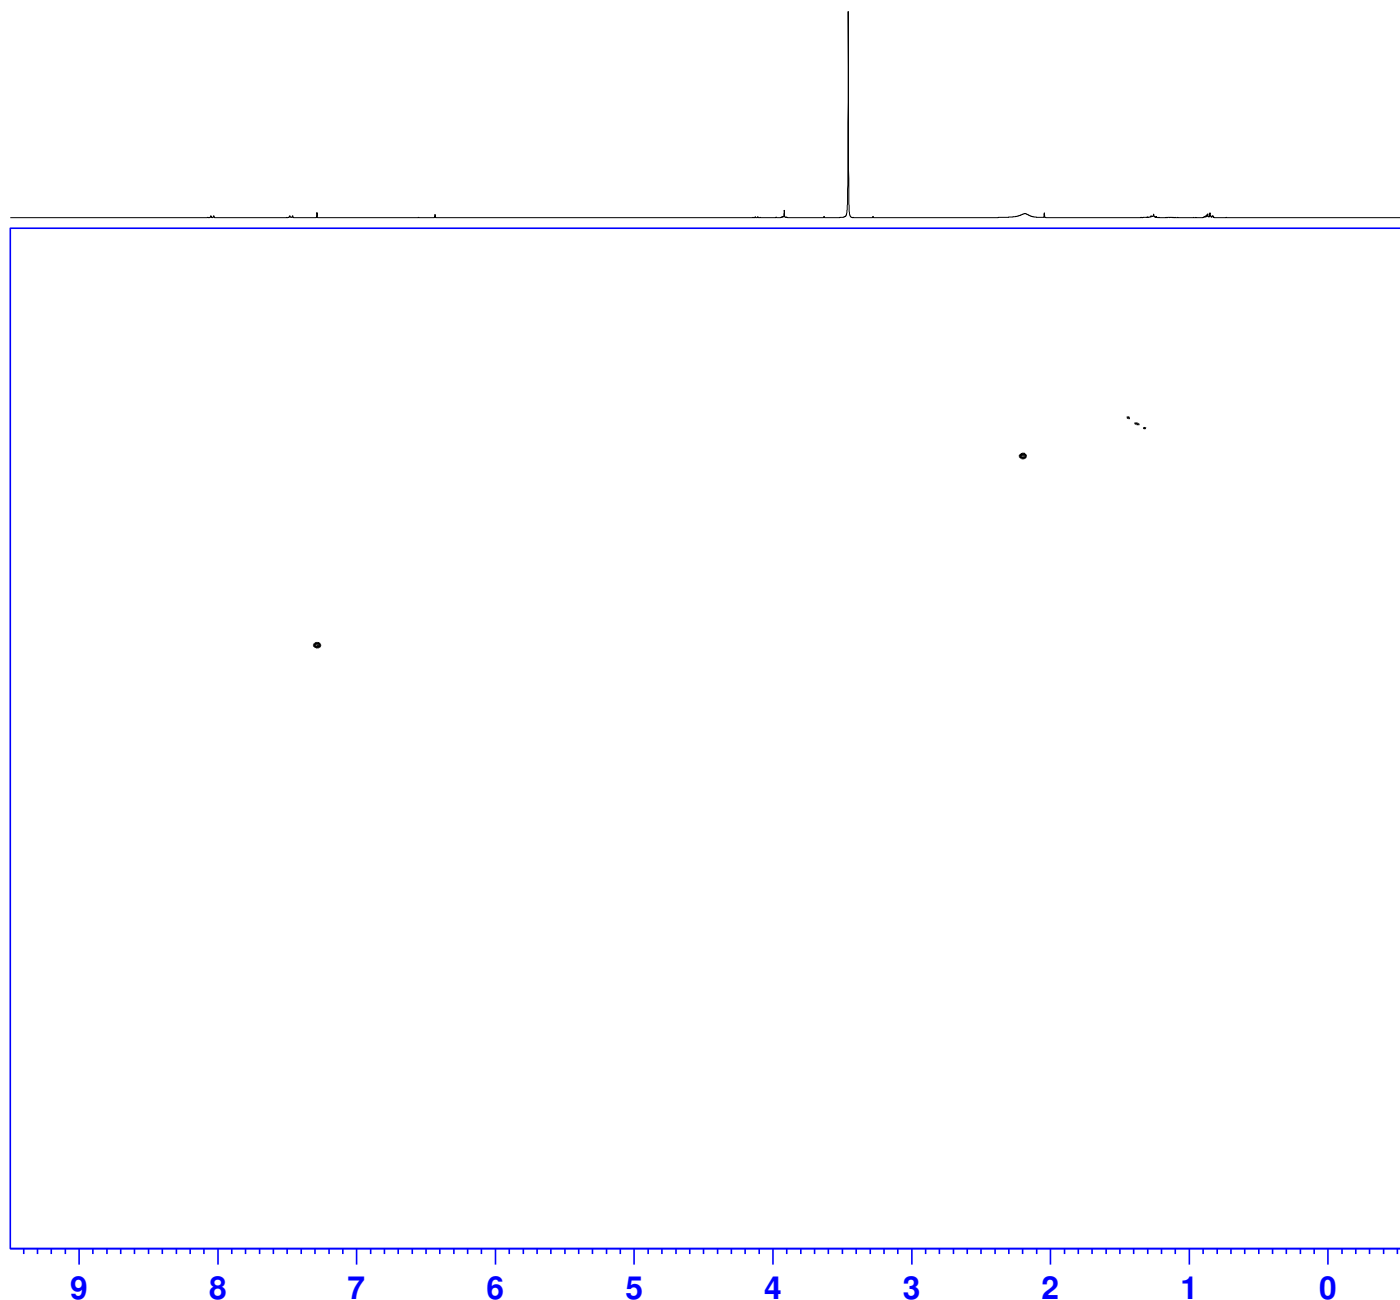

F2 - Acquisition Parameters  
Date\_ 20220918  
Time 19.03 h  
INSTRUM spect  
PROBHD Z108618\_1022 (  
PULPROG hmqcgpgf  
TD 1152  
SOLVENT CDC13  
NS 24  
DS 16  
SWH 4032.258 Hz  
FIDRES 7.000448 Hz  
AQ 0.1428480 sec  
RG 198.49  
DW 124.000 usec  
DE 6.50 usec  
TE 298.4 K  
CNST2 145.0000000  
D0 0.00000300 sec  
D1 1.50000000 sec  
D2 0.00344828 sec  
D12 0.00002000 sec  
D13 0.00000400 sec  
D16 0.00020000 sec  
IN0 0.00001990 sec  
TDav 1  
SFO1 400.1317832 MHz  
NUC1 1H  
P1 14.00 usec  
P2 28.00 usec  
PLW1 14.03100014 W  
SFO2 100.6228298 MHz  
NUC2 13C  
CPDPRG[2] garp  
P3 10.00 usec  
PCPD2 80.00 usec  
PLW2 60.64099884 W  
PLW12 0.94751000 W  
GPNAM[1] SMSQ10.100  
GPZ1 50.00 %  
GPNAM[2] SMSQ10.100  
GPZ2 30.00 %  
GPNAM[3] SMSQ10.100  
GPZ3 40.10 %  
P16 1000.00 usec  
  
F1 - Acquisition parameters  
TD 256  
SFO1 100.6228 MHz  
FIDRES 196.293976 Hz  
SW 249.701 ppm  
FnMODE QF  
  
F2 - Processing parameters  
SI 1024  
SF 400.1300000 MHz  
WDW QSINE  
SSB 2  
LB 0 Hz  
GB 0  
PC 1.40  
  
F1 - Processing parameters  
SI 1024  
MC2 QF  
SF 100.6127685 MHz  
WDW QSINE  
SSB 2  
LB 0 Hz  
GB 0