

ZP\_COSYGPSW\_30min DMSO {C:\Bruker\TopSpin3.6.5} AMP 14




Current Data Parameters  
NAME CCY\_150\_02-All-Check2  
EXPNO 14  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20231106  
Time 6.51 h  
INSTRUM spect  
PROBHD Z108618\_1022 (  
PULPROG cosygpppqf  
TD 2048  
SOLVENT DMSO  
NS 16  
DS 16  
SWH 4672.897 Hz  
FIDRES 4.563376 Hz  
AQ 0.2191360 sec  
RG 154.8  
DW 107.000 usec  
DE 6.50 usec  
TE 298.1 K  
D0 0.00000300 sec  
D1 1.90702105 sec  
D11 0.03000000 sec  
D12 0.00002000 sec  
D13 0.00000400 sec  
D16 0.00020000 sec  
IN0 0.00021400 sec  
TDav 1  
SF01 400.1319696 MHz  
NUC1 1H  
P0 14.00 usec  
P1 14.00 usec  
P17 2500.00 usec  
PLW1 15.09500027 W  
PLW10 3.28730011 W  
GPNAM[1] SMSQ10.100  
GPZ1 10.00 %  
P16 1000.00 usec

F1 - Acquisition parameters  
TD 128  
SF01 400.132 MHz  
FIDRES 73.014015 Hz  
SW 11.678 ppm  
FnMODE QF

F2 - Processing parameters  
SI 1024  
SF 400.1300016 MHz  
WDW QSINE  
SSB 0  
LB 0 Hz  
GB 0  
PC 1.40

F1 - Processing parameters  
SI 1024  
MC2 QF  
SF 400.1300016 MHz  
WDW QSINE  
SSB 0  
LB 0 Hz  
GB 0

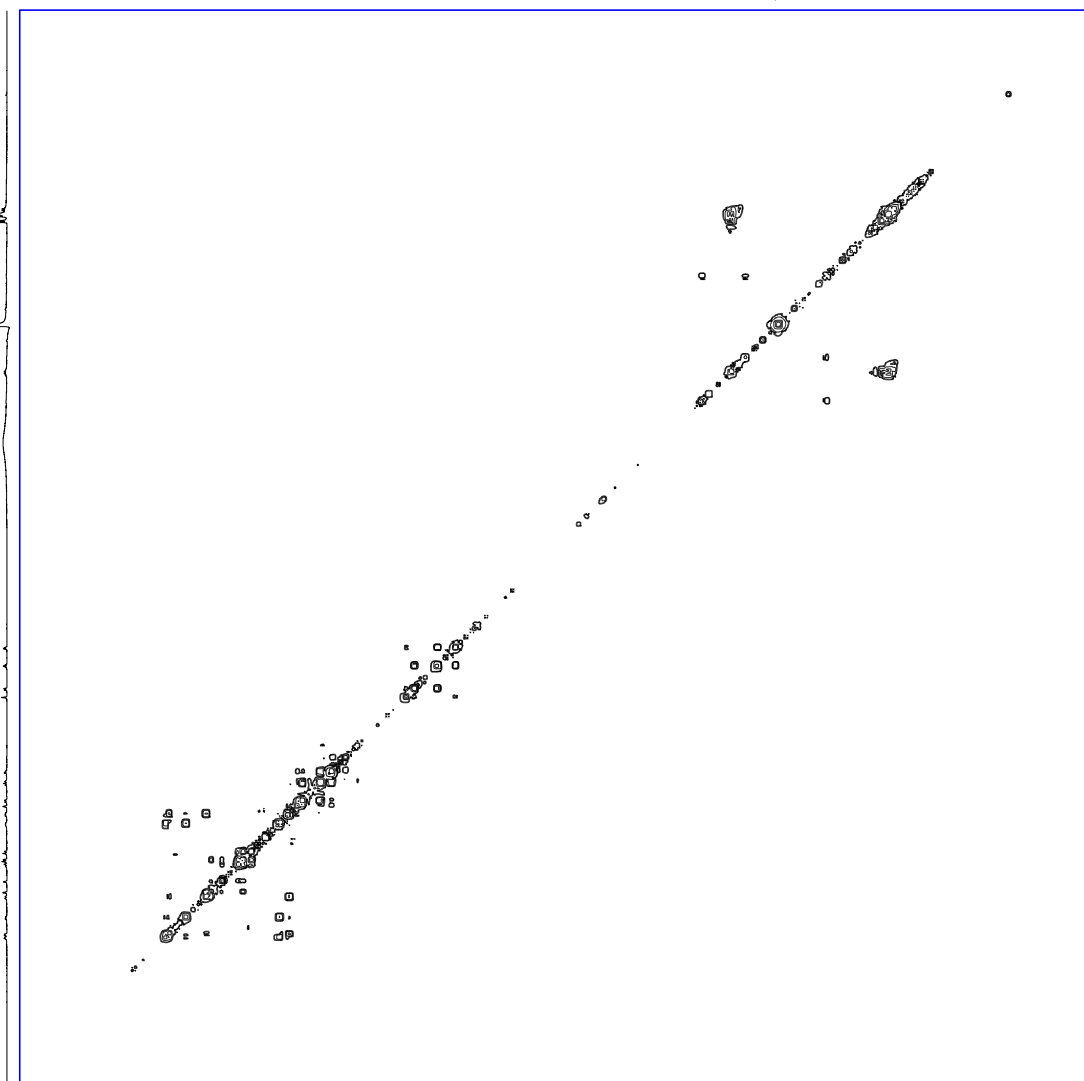

ppm

0

1

2

3

4

5

6

7

8

9

10

ppm